

FIG.1

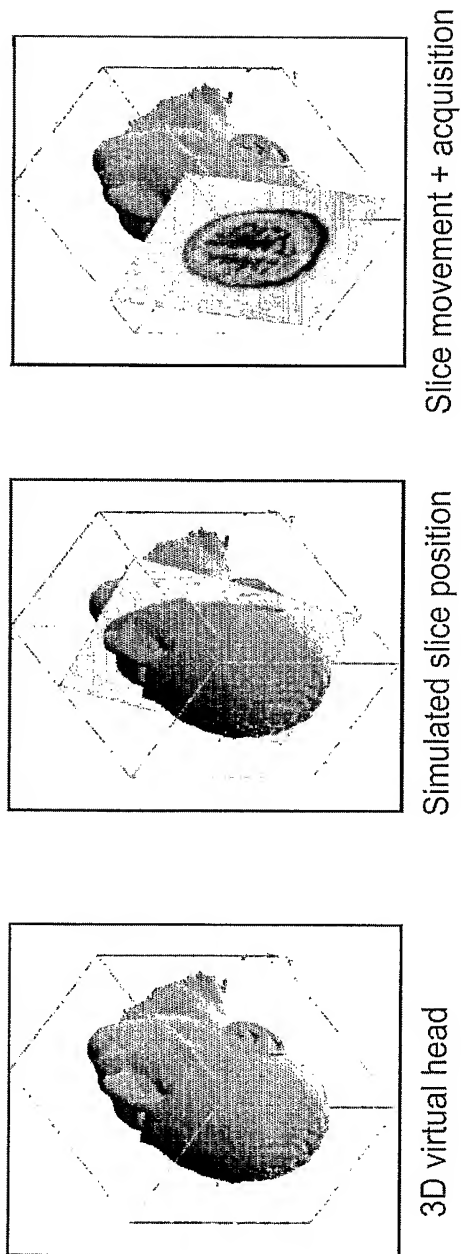


FIG.2

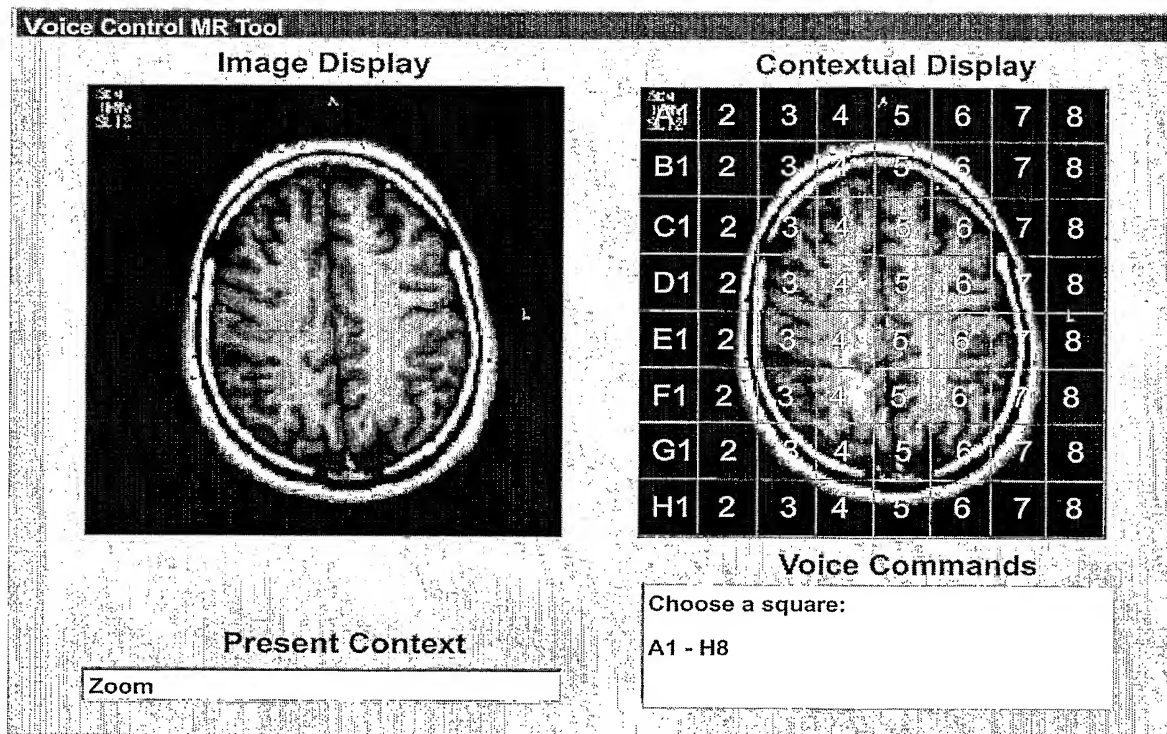


FIG.3

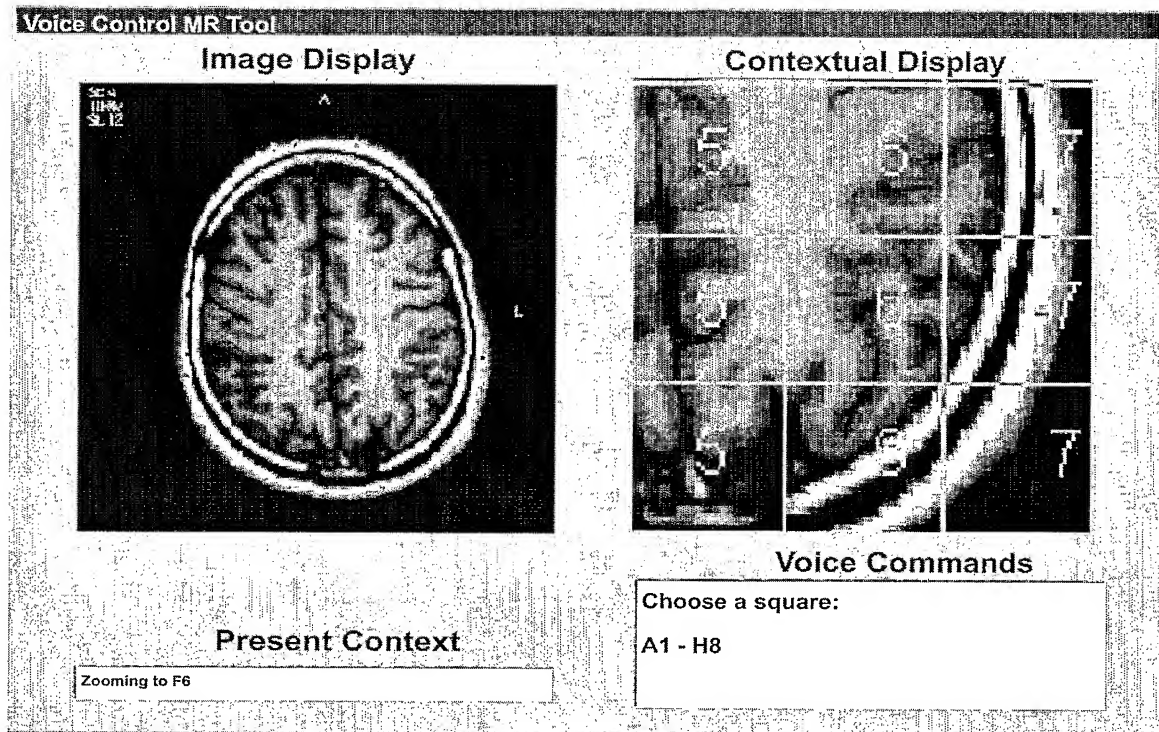


FIG.4

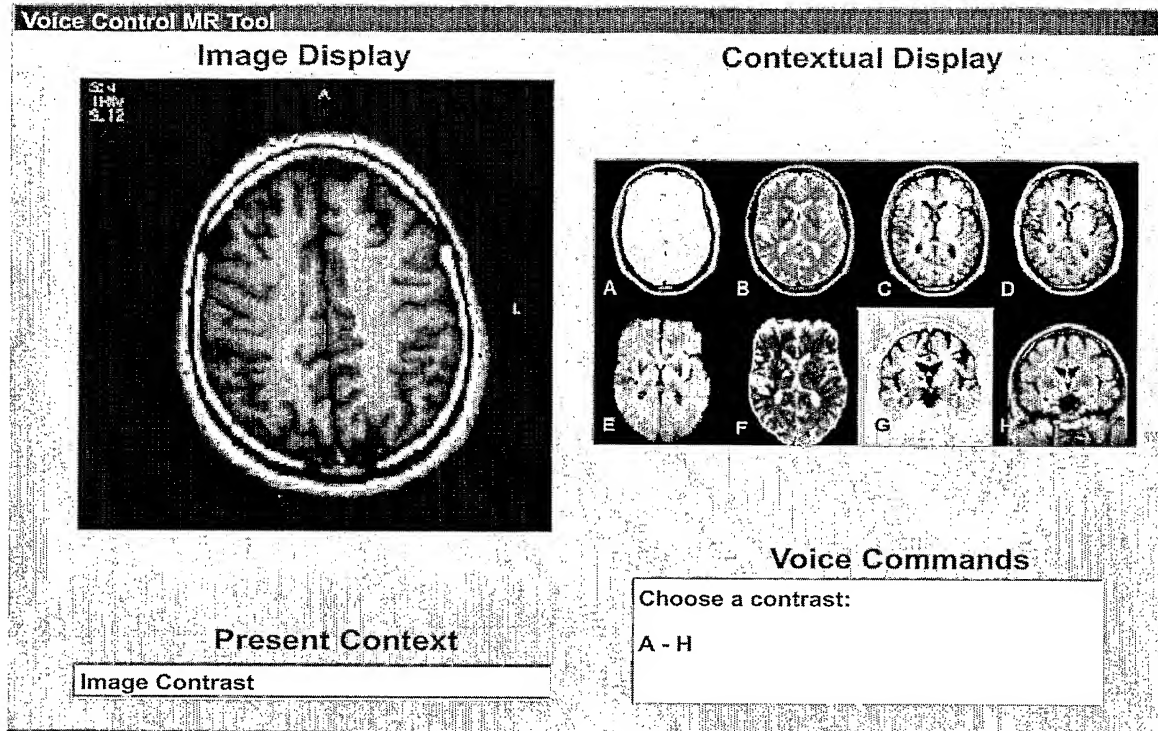


FIG.5

Method	Acquisition time	Relative acquisition %
EPI	50 ms	1%
SS-TSE	300 ms	6%
TSE	60 seconds	200 %
SE	120 seconds	400 %

FIG.6

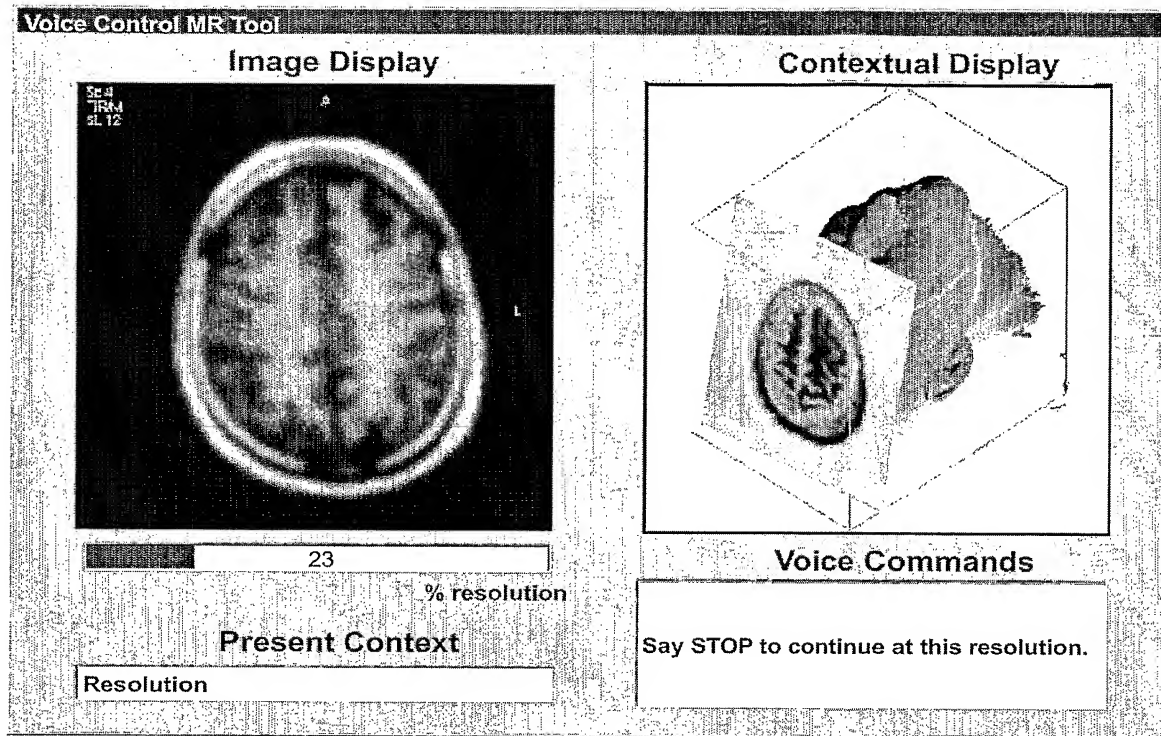


FIG.7

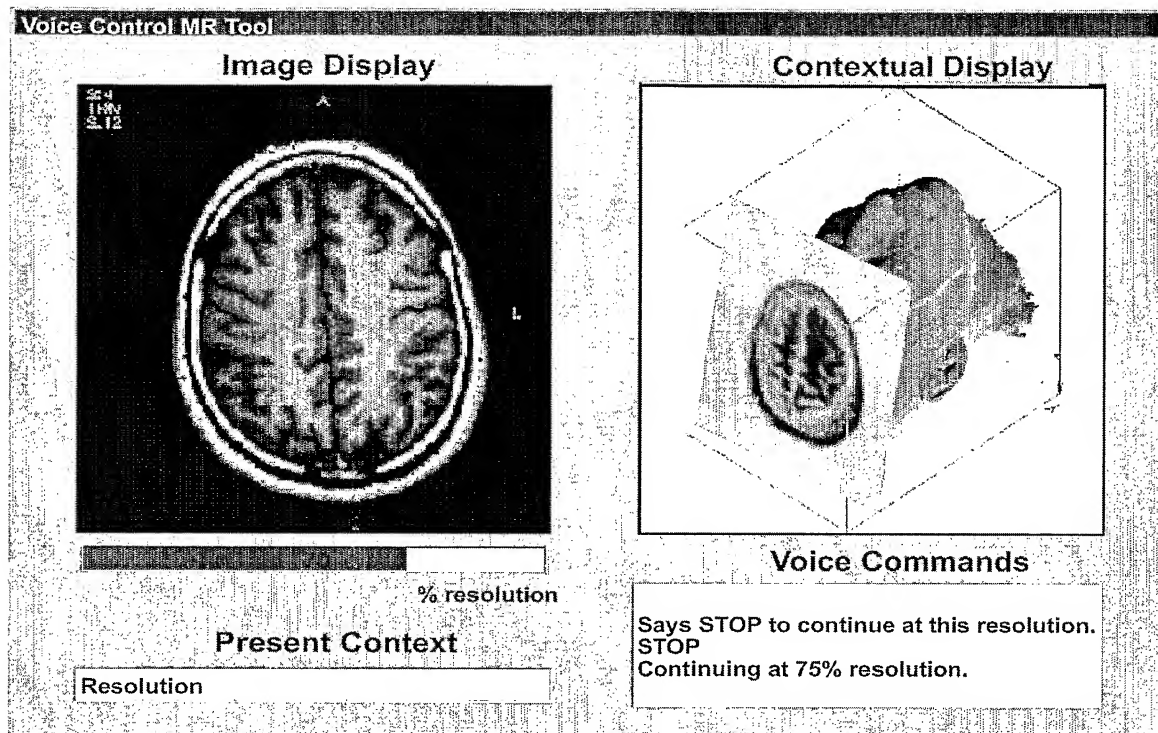


FIG.8